


Freedom from Long-Term Polymer Exposure




✓

SYNERGY™ Stent offers peace of mind knowing that the polymer is gone shortly after the drug is completely eluted at 3 months¹

Synchronous Drug Elution and Polymer Absorption

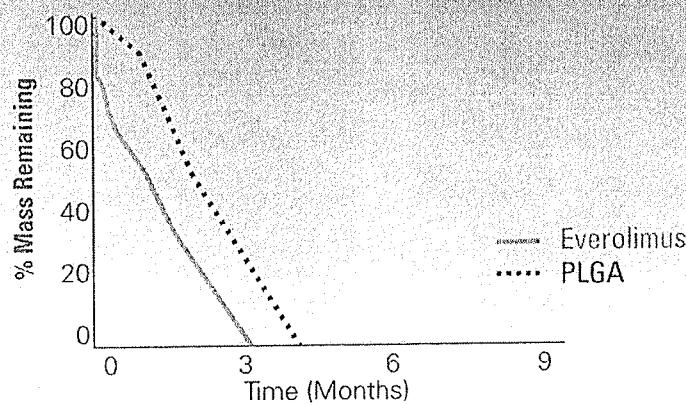

Polymer Absorption Rates in Perspective

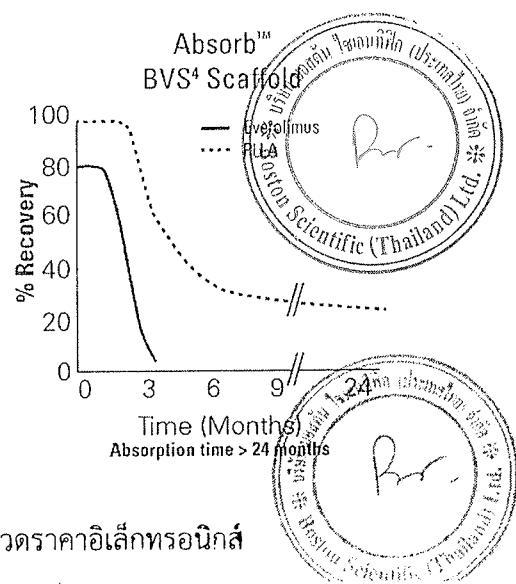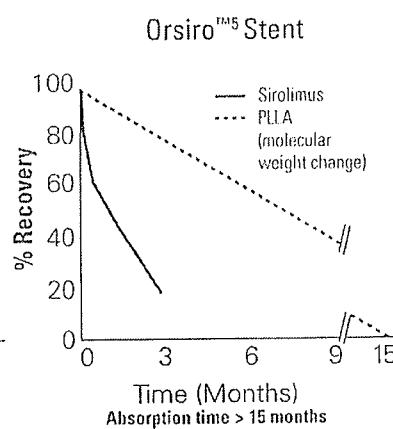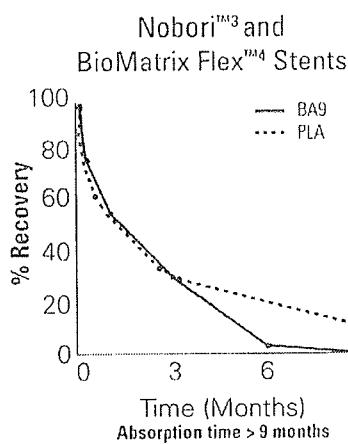

คณะกรรมการพิจารณาผลการประกวดราคากลางท้องถิ่นสํา

๑.ลงชื่อ.....*เจตนา*.....ประธานกรรมการ

๒.ลงชื่อ.....*บดินทร์*.....กรรมการ

๓.ลงชื่อ.....*ทวีวรรณ*.....กรรมการ

๔.ลงชื่อ.....*กรรณา*.....กรรมการ

EVOLVE III Clinical Trial


SYNERGY™ STENT

**Broadest and most complex patient population
ever studied in a U.S. Pivotal Trial**


EVOLVE III Clinical Trial Study Overview

Patients (1,684) were randomized 1:1 to SYNERGY or PROMUS Element™ Plus Stent Systems with <9 native coronary artery lesions in <2 major epicardial vessels, lesion length ≤34 mm, RVD = 2.25 to ≤4.0 mm, %DS = 50 to ≤100 (excluded LM disease, SVG, CTO, or recent STEMI)

EVOLVE II Clinical Trial A More Comers Study⁴

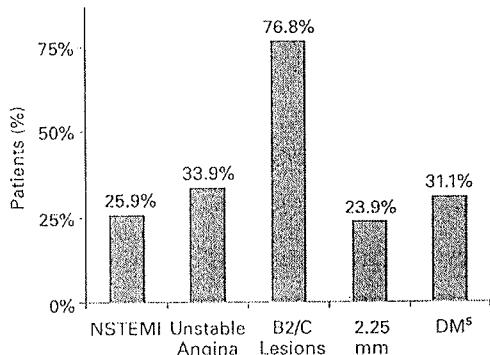


Primary Endpoint of Target Lesion Failure⁶ (TLF) Met

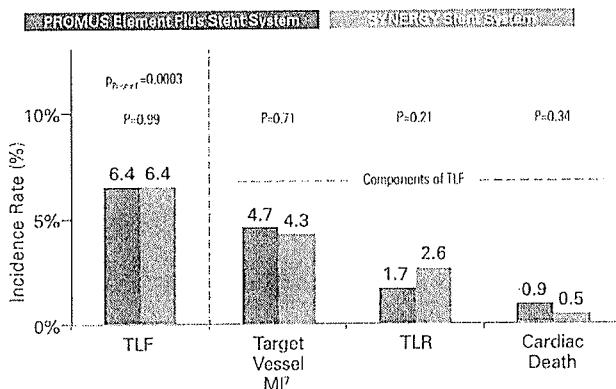

ZERO definite ST events in SYNERGY arm after 24 hours⁴

Stent Thrombosis (ST) (Definite/Probable) Through 12 Months⁴

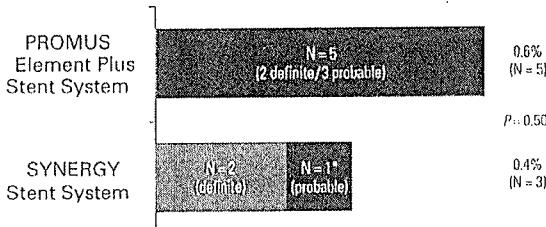

*Occurred on day 6. ST rates were equivalent when analyzed in an intent-to-treat or per protocol manner.

Adult (≥1 day) Sub-Acute (2–30 days) Late (31–180 days) 181+ days



4. EVOLVE II Clinical Trial presented by Dean Kereiakes, MD at AHA 2014. 1,694 patients were randomized 1:1 to SYNERGY or PROMUS Element™ Plus Stent Systems. Graph shows TLF Per Protocol (PP) and MI, TLR, CD shown for the Intent-to-Treat (ITT) population. ITT TLF for SYNERGY Stent = 6.7% and for PROMUS Element Stent = 6.4%, respectively ($p=0.0005$ for non-inferiority). The SYNERGY Stent is an investigational device and not for sale in the U.S. or Japan.

5. Medically-Treated Diabetes Mellitus

6. IU: ischemia-driven TLR, MI related to the target vessel, or any cardiac death. To conclude non-inferiority, the primary endpoint was required to have been met in both intent-to-treat and per protocol patient populations.

7. Per protocol spontaneous MI is defined as rise and/or fall of cardiac biomarkers with one value >95th percentile of the UHL + with evidence of myocardial ischemia. Per-PCI MI is defined as one of the following: i) ECG elevations within 48 hours of PCI (based on CK-MB >3X URL), ii) new pathological Q waves, or iii) autopsy evidence of acute MI.

8. Meredith T, AM, MBBS, PhD, PCR 2014. Only the "full dose" SYNERGY Stent results are shown.



คณะกรรมการพิจารณาผลการประกวดราคากลีกทรอนิกส์

๑.ลงชื่อ.....กานต์ พัฒนา.....ประธานกรรมการ

๒.ลงชื่อ.....กานต์ พัฒนา.....กรรมการ

๓.ลงชื่อ.....กานต์ พัฒนา.....กรรมการ


EVOLVE Clinical Trial

SYNERGY™ STENT


Outstanding Safety and Efficacy at 3-Years

Early and long-term data demonstrates exceptional results.⁸



0% TLR from 6 Months to 3-Years⁸

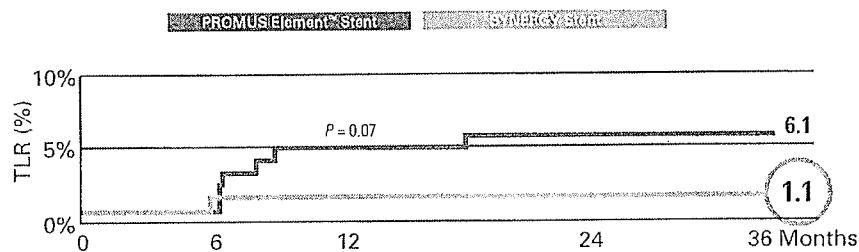

1.1% TLR and 0% ARC ST at 3-Years⁸

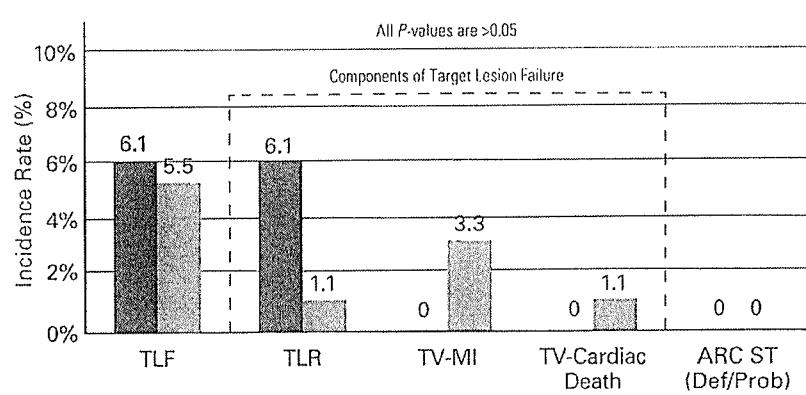

One NSTEMI in the SYNERGY group was periprocedural. The remaining 2 NSTEMI in the SYNERGY arm were considered unrelated to the study device: one at day 347 due to anemia and a major GI bleed, and one at day 364 subsequent to respiratory failure in a patient with severe COPD—enzymes were checked indicating that a NSTEMI had occurred. The one death was of an unknown cause at day 472 and adjudicated as a Cardiac Death. Safety Population.



คณะกรรมการพิจารณาผลการประมวลผลทางการแพทย์ของประเทศไทย


๑. ลงชื่อ..... *GLAY* ประธานกรรมการ

๒. ลงชื่อ..... *ท. พัฒน์* กรรมการ

๓. ลงชื่อ..... *วันรุ่งไวยา* กรรมการ

SYNERGY™ Stent Clinical Program and Research*

Addressing full spectrum of cardiovascular disease complexity

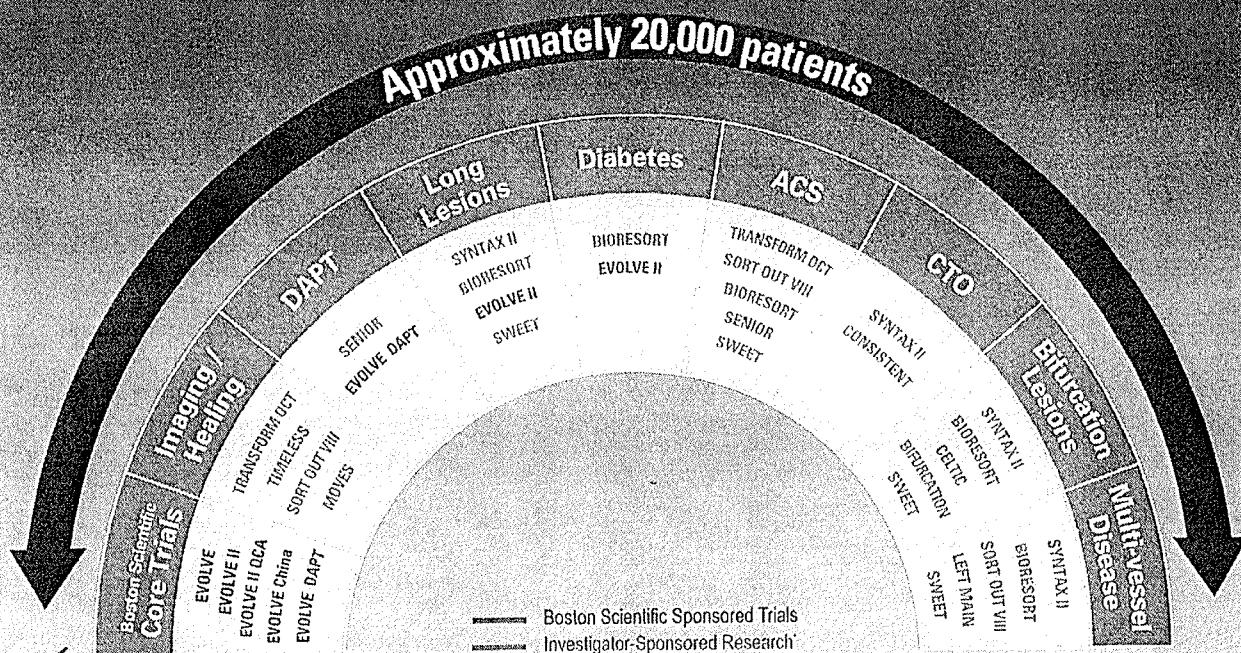

SYNERGY Everolimus-Eluting Platinum Chromium Coronary Stent System

MONORAIL™ CATHETER—PRODUCT ORDERING INFORMATION

Ø (mm)	STENT LENGTH (mm)								Overexpansion Capabilities
	8	12	16	20	24	28	32	38	
2.0	H7493926218220	H7493926212220	H7493926216220	H7493926220220	H7493926224220	H7493926228220	H7493926324220	H7493926328220	3.50
2.50	H7493926208250	H7493926212250	H7493926216250	H7493926220250	H7493926224250	H7493926228250	H7493926232250	H7493926238250	3.50
2.75	H7493926203270	H7493926212270	H7493926216270	H7493926220270	H7493926224270	H7493926228270	H7493926324270	H7493926328270	3.60
3.00	H7493926208300	H7493926212300	H7493926216300	H7493926220300	H7493926224300	H7493926228300	H7493926232300	H7493926238300	4.25
3.50	H7493926203350	H7493926212350	H7493926216350	H7493926220350	H7493926224350	H7493926228350	H7493926324350	H7493926328350	4.25
4.00	H7493926208400	H7493926212400	H7493926216400	H7493926220400	H7493926224400	H7493926228400	H7493926232400	H7493926238400	5.75

* Boston Scientific is not responsible for the collection, analysis or reporting of the investigator-sponsored research output which is the sole responsibility of the investigators. Boston Scientific's involvement in investigator-sponsored research is limited to providing financial support for research that advances medical and scientific knowledge about our products.

CAUTION: The law restricts these devices to sale by or on the order of a physician. Indications, contraindications, warnings and instructions for use can be found in the product labelling supplied with each device. Information for the use only in countries with applicable health authority product registrations. Information contained herein is for distribution outside the US, France, and Japan only.

All cited trademarks are the property of their respective owners.

Boston
Scientific

Advancing science for life™

bostonscientific-international.com


© 2014 Boston Scientific Corporation
or its affiliates. All rights reserved.
IC-222116-AD NOV2014

คณบดีกรรมการพิจารณาผลการประกวดราคาอิเล็กทรอนิกส์

๑.ลงชื่อ.....
.....
.....

๒.ลงชื่อ.....
.....
.....

๓.ลงชื่อ.....
.....
.....



.....
.....
.....