

ZERTIFIKAT ◆ CERTIFICATE ◆ 認證書 ◆ CERTIFICADO ◆ CERTIFIKAT ◆ CERTIFICATE



America

CERTIFICATE

No. QS2 089344 0003 Rev. 01

Certificate Holder: **Nipro Sales (Thailand) Co., Ltd.**
89/170 Nipro Building
Viphavadee Rangsit Road
Talad Bangkhen, Laksi
Bangkok 10210
THAILAND

Certification Mark:



Scope of Certificate: **Storage and Distribution of Sterile and Non-Sterile Single Use Medical Products for Cardiopulmonary Bypass Surgery, Hemodialysis, Infusion, Injection, Adhesive Bandages, Lancets and Lancing Devices**


Standard: **ISO 13485:2016**

The Certification Body of TÜV SÜD America Inc. certifies that the company mentioned above has established and is maintaining a quality management system that meets the requirements of the listed standards.

Report No.: **TH0161020T156**

Effective Date: **2021-02-13**

Expiry Date: **2024-02-12**

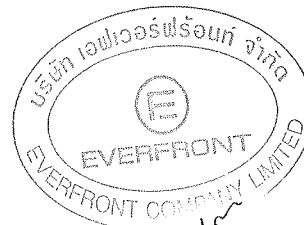

Page 1 of 1

Date of Issue: 2021-01-29

(Tina Israel)
Manager, US Certification Body,
Medical and Health Services



NIPRO (THAILAND) CORPORATION LIMITED
10/2 MOO 8 BANGHON KO, SENA PHRA NAKHON SI AYUTTHAYA 13110, THAILAND
TEL: +86-35-201818 FAX: +86-35-201625

CERTIFICATE

PRODUCT NAME : PACK NEEDLE


SIZE : 18Gx1 1/2" L.R.TW.E.P.ISO TH

DATE : 5 Aug. 2022

LOT NO. : 22E26


QUALITY CONTROL NO. 2 SECTION

TEST ITEM	UNIT	SPECIFICATION	RESULT
EXTRACTION TEST			
Limit degree of acid and alkalinity		Within 1 unit of pH	0.04
Limit of elution metal			
- Total amount of Pb, Zn, Fe, Sn	mg/L	Not greater than 5	0.0058
- Cd	mg/L	Less than 0.1	0.0000
CORROSION RESISTANCE TEST			
		No Sign of corrosion	No Sign of corrosion
LUBRICANT	mg/cm ²	Not exceed 0.25	0.019
JUDGEMENT : PASSED			
TEST METHOD : ISO 7864 : 2016 " Sterile hypodermic needles for single use "			
ISO 9626 : 2016 " Stainless steel needles tubing for manufacture of medical devices"			

Approved by : 

(Ms.Pilmphijit B.)

Quality Control No.2 Section Manager

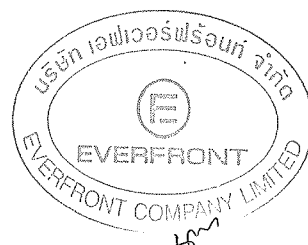



NIPRO (THAILAND) CORPORATION LIMITED
 10/2 MOO 8 BANGNOMKO, SENAPHRA NAKHON SIAYUTTHAYA 13110, THAILAND
 TEL: +66-35-201618 FAX: +66-35-201626

CERTIFICATE

PRODUCT NAME : PACK NEEDLE


SIZE : 20Gx1 1/2" L.R.TW.E.P.ISO TH

DATE : 5 Aug. 2022

LOT NO. : 22E21

QUALITY CONTROL NO. 2 SECTION


TEST ITEM	UNIT	SPECIFICATION	RESULT
<u>EXTRACTION TEST</u>			
Limit degree of acid and alkalinity		Within 1 unit of pH	0.05
Limit of elution metal			
- Total amount of Pb, Zn, Fe, Sn	mg/L	Not greater than 5	0.0000
- Cd	mg/L	Less than 0.1	0.0009
<u>CORROSION RESISTANCE TEST</u>			
<u>LUBRICANT</u>	mg/cm^2	No Sign of corrosion Not exceed 0.25	No Sign of corrosion 0.035
JUDGEMENT :		PASSED	
<p>TEST METHOD : ISO 7864 : 2016 " Sterile hypodermic needles for single use " ISO 9626 : 2016 " Stainless steel needles tubing for manufacture of medical devices "</p>			



Approved by:

(Ms. Phimphijit B.)

Quality Control No.2 Section Manager

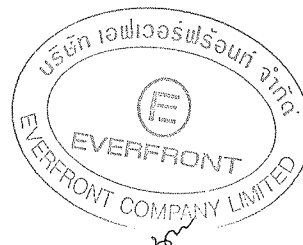



NIPRO (THAILAND) CORPORATION LIMITED
10/2 MOO 8 BANGHOMIKO, SENAI PHRA NAKHON SIAYUTTHAYA : 3110, THAILAND
TEL: +86-36-201618 FAX: +86-36-201626

CERTIFICATE

PRODUCT NAME : PACK NEEDLE


SIZE : 21Gx1 1/2" LR.TW.E.P.ISO TH

DATE : 28 Apr. 2022

LOT NO. : 22B07

QUALITY CONTROL NO. 2 SECTION


TEST ITEM	UNIT	SPECIFICATION	RESULT
EXTRACTION TEST			
Limit degree of acid and alkalinity		Within 1 unit of pH	0.07
Limit of elution metal			
- Total amount of Pb, Zn, Fe, Sn	mg/L	Not greater than 5	0.0003
- Cd	mg/L	Less than 0.1	0.0000
CORROSION RESISTANCE TEST			
		No Sign of corrosion	No Sign of corrosion
LUBRICANT	mg/cm ²	Not exceed 0.25	0.019
JUDGEMENT : PASSED			
TEST METHOD : ISO 7864 : 2016 " Sterile hypodermic needles for single use " ISO 9626 : 2016 " Stainless steel needles tubing for manufacture of medical devices "			

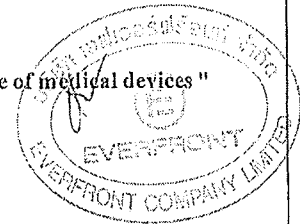

Approved by : _____

(Ms. Phimpijit B.)

Quality Control No.2 Section Manager

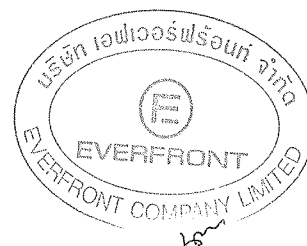



NIPRO (THAILAND) CORPORATION LIMITED
10/2 MOO 8 BANGNOMKO, SENAPHRA NAKHON SIAYUTTHAYA 13110, THAILAND
TEL: +66-35-201818 FAX: +66-35-201625

CERTIFICATE

PRODUCT NAME : PACK NEEDLE


SIZE : 21Gx1" LR.TW.E.P.ISO TH


DATE : 5 Aug. 2022

LOT NO. : 22F20

QUALITY CONTROL NO. 2 SECTION


TEST ITEM	UNIT	SPECIFICATION	RESULT
<u>EXTRACTION TEST</u>			
Limit degree of acid and alkalinity		Within 1 unit of pH	0.05
Limit of elution metal			
- Total amount of Pb, Zn, Fe, Sn	mg/L	Not greater than 5	0.0001
- Cd	mg/L	Less than 0.1	0.0000
<u>CORROSION RESISTANCE TEST</u>			
		No Sign of corrosion	No Sign of corrosion
<u>LUBRICANT</u>	mg/cm ²	Not exceed 0.25	0.055
JUDGEMENT :		PASSED	
TEST METHOD : ISO 7864 : 2016 " Sterile hypodermic needles for single use " ISO 9626 : 2016 " Stainless steel needles tubing for manufacture of medical devices "			



Approved by : 

(Ms. Phimphijit B.)

Quality Control No.2 Section Manager

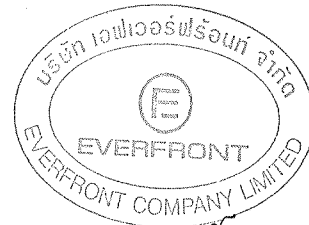

16



NIPRO (THAILAND) CORPORATION LIMITED
10/2 MOO 8 BANGHOMIKO, SENI, PHRA NAKHON SIAYUTTHAYA 13110, THAILAND
TEL: +66-35-201618 FAX: +66-35-201629

CERTIFICATE

PRODUCT NAME : PACK NEEDLE


SIZE : 22Gx1" LR.TW.E.P.ISO TH

DATE : 5 Aug. 2022

LOT NO. : 22F21


QUALITY CONTROL NO. 2 SECTION

TEST ITEM	UNIT	SPECIFICATION	RESULT
<u>EXTRACTION TEST</u>			
Limit degree of acid and alkalinity		Within 1 unit of pH	0.10
Limit of elution metal			
- Total amount of Pb, Zn, Fe, Sn	mg/L	Not greater than 5	0.0000
- Cd	mg/L	Less than 0.1	0.0013
<u>CORROSION RESISTANCE TEST</u>			
		No Sign of corrosion	No Sign of corrosion
<u>LUBRICANT</u>	mg/cm ²	Not exceed 0.25	0.027
JUDGEMENT :	PASSED		
TEST METHOD : ISO 7864 : 2016 " Sterile hypodermic needles for single use " ISO 9626 : 2016 " Stainless steel needles tubing for manufacture of medical devices "			

Approved by : 

(Ms. Phimphijit B.)

Quality Control No.2 Section Manager

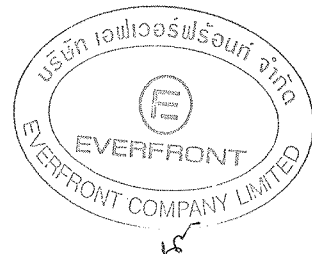



NIPRO

NIPRO (THAILAND) CORPORATION LIMITED
10/2 MOO 8 BANGNOMKIC, SENA PHRA NAKHON SIAYUTTHAYA 13110, THAILAND
TEL: +86-35-201818 FAX: +86-35-201625

CERTIFICATE

PRODUCT NAME : PACK NEEDLE


SIZE : 22Gx1 1/2" LR.TW.E.P.ISO TH

DATE : 5 Aug. 2022

LOT NO. : 22F05

QUALITY CONTROL NO .2 SECTION


TEST ITEM	UNIT	SPECIFICATION	RESULT
<u>EXTRACTION TEST</u>			
Limit degree of acid and alkalinity		Within 1 unit of pH	0.10
Limit of elution metal			
- Total amount of Pb, Zn, Fe, Sn	mg/L	Not greater than 5	0.0000
- Cd	mg/L	Less than 0.1	0.0013
<u>CORROSION RESISTANCE TEST</u>			
		No Sign of corrosion	No Sign of corrosion
<u>LUBRICANT</u>	mg/cm ²	Not exceed 0.25	0.027
JUDGEMENT :		PASSED	
TEST METHOD : ISO 7864 : 2016 " Sterile hypodermic needles for single use "			
ISO 9626 : 2016 " Stainless steel needles tubing for manufacture of medical devices "			



Approved by : _____

(Ms.Phimpijit B.)

Quality Control No.2 Section Manager

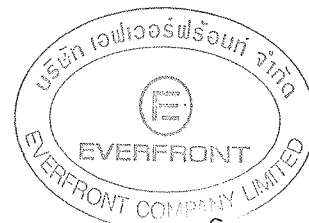



NIPRO (THAILAND) CORPORATION LIMITED
10/2 MOO 8 BANGHOMKO, SENA, PHRA NAKI ION SIAYUTTHAYA 13110, THAILAND
TEL: +66-35-201618 FAX: +66-35-201625

CERTIFICATE

PRODUCT NAME : PACK NEEDLE


SIZE : 23Gx1" LR.TW.E.P.ISO TH


DATE : 5 Aug. 2022

LOT NO. : 22F08

QUALITY CONTROL NO. 2 SECTION


TEST ITEM	UNIT	SPECIFICATION	RESULT
EXTRACTION TEST			
Limit degree of acid and alkalinity		Within 1 unit of pH	0.04
Limit of elution metal			
- Total amount of Pb, Zn, Fe, Sn	mg/L	Not greater than 5	0.0000
- Cd	mg/L	Less than 0.1	0.0023
CORROSION RESISTANCE TEST			
		No Sign of corrosion	No Sign of corrosion
LUBRICANT	mg/cm ²	Not exceed 0.25	0.039
JUDGEMENT :		PASSED	
TEST METHOD : ISO 7864 : 2016 " Sterile hypodermic needles for single use " ISO 9626 : 2016 " Stainless steel needles tubing for manufacture of medical devices "			

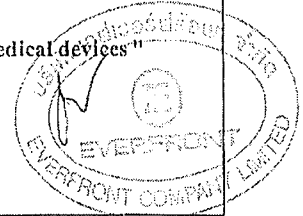

Approved by : 

(Ms. Phimpijit B.)

Quality Control No.2 Section Manager

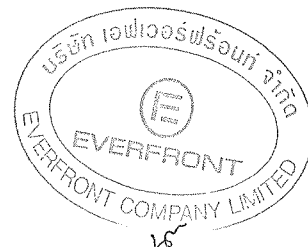



NIPRO (THAILAND) CORPORATION LIMITED
10/2 MOO 8 BANGHOKKO,SENA,PHRA NAKH ION SI AYUTTHAIYA 13110,THAILAND
TEL: +66-36-201818 FAX: +66-36-201825

CERTIFICATE

PRODUCT NAME : PACK NEEDLE


SIZE : 23Gx1 1/2" LR.TW.E.P.ISO TH


DATE : 15 Jun. 2022

LOT NO. : 22D08

QUALITY CONTROL NO. 2 SECTION


TEST ITEM	UNIT	SPECIFICATION	RESULT
<u>EXTRACTION TEST</u>			
Limit degree of acid and alkalinity		Within 1 unit of pH	0.19
Limit of elution metal			
- Total amount of Pb, Zn , Fe, Sn	mg/L	Not greater than 5	0.0000
- Cd	mg/L	Less than 0.1	0.0000
<u>CORROSION RESISTANCE TEST</u>			
		No Sign of corrosion	No Sign of corrosion
<u>LUBRICANT</u>	mg/cm ²	Not exceed 0.25	0.036
JUDGEMENT : PASSED			
TEST METHOD : ISO 7864 : 2016 " Sterile hypodermic needles for single use " ISO 9626 : 2016 " Stainless steel needles tubing for manufacture of medical devices "			

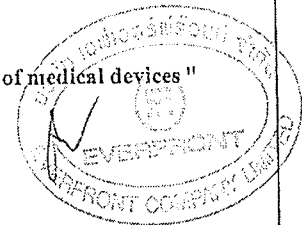

Approved by : 

(Ms.Phimphijit B.)

Quality Control No.2 Section Manager

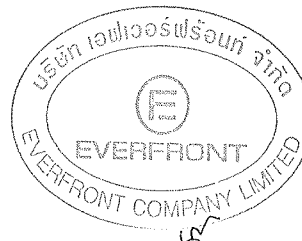



NIPRO (THAILAND) CORPORATION LIMITED
10/2 MOO 8 BANGHOMKO, SENA, PHRA NAKH ION SIAYUTTHIAYA 13110, THAILAND
TEL: +66-35-201818 FAX: +66-35-201625

CERTIFICATE

PRODUCT NAME : PACK NEEDLE


SIZE : 24Gx1" LR.TW.E.P.ISO (TH)

DATE : 19 Jul. 2022

LOT NO. : 22E16, 22E17


QUALITY CONTROL NO. 2 SECTION

TEST ITEM	UNIT	SPECIFICATION	RESULT
<u>EXTRACTION TEST</u>			
Limit degree of acid and alkalinity		Within 1 unit of pH	0.17
Limit of elution metal			
- Total amount of Pb, Zn, Fe, Sn	mg/L	Not greater than 5	0.0034
- Cd	mg/L	Less than 0.1	0.0000
<u>CORROSION RESISTANCE TEST</u>			
		No Sign of corrosion	No Sign of corrosion
<u>LUBRICANT</u>	mg/cm ²	Not exceed 0.25	0.032
JUDGEMENT : PASSED			
TEST METHOD : ISO 7864 : 2016 " Sterile hypodermic needles for single use " ISO 9626 : 2016 " Stainless steel needles tubing for manufacture of medical devices "			

Approved by : 

(Ms. Phinphijit B.)

Quality Control No.2 Section Manager

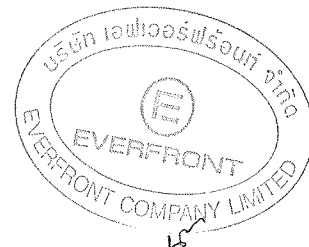



NIPRO (THAILAND) CORPORATION LIMITED
 10/2 MOO 8 BANGHONKHO, SENA PHRA NAKH ION SI AYUTTHAYA 13110, THAILAND
 TEL: +66-35-201818 FAX: +66-35-201626

CERTIFICATE

PRODUCT NAME : PACK NEEDLE


SIZE : 24Gx1 1/2" LR, TW, E.P. ISO TH

DATE : 19 Jul. 2022

LOT NO. : 22E19

QUALITY CONTROL NO. 2 SECTION


TEST ITEM	UNIT	SPECIFICATION	RESULT
<u>EXTRACTION TEST</u>			
Limit degree of acid and alkalinity		Within 1 unit of pH	0.17
Limit of elution metal			
- Total amount of Pb, Zn, Fe, Sn	mg/L	Not greater than 5	0.0034
- Cd	mg/L	Less than 0.1	0.0000
<u>CORROSION RESISTANCE TEST</u>			
		No Sign of corrosion	No Sign of corrosion
<u>LUBRICANT</u>	mg/cm ²	Not exceed 0.25	0.032
JUDGEMENT :		PASSED	
<p>TEST METHOD : ISO 7864 : 2016 " Sterile hypodermic needles for single use " ISO 9626 : 2016 " Stainless steel needles tubing for manufacture of medical devices "</p>			



Approved by :

(Ms. Phimpijit B.)

Quality Control No.2 Section Manager

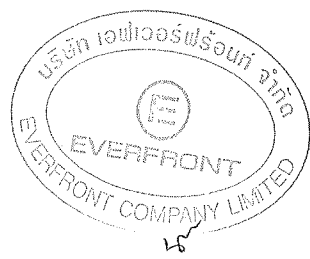



NIPRO (THAILAND) CORPORATION LIMITED
 10/2 MOO 8 BANGHOMKO,SENA,PHRA NAKHON SI AYUTTHAYA 13110,THAILAND
 TEL: +66-35-201618 FAX: +66-35-201625

CERTIFICATE

PRODUCT NAME : PACK NEEDLE


SIZE : 25Gx1" LR.TW.E.P.ISO TH

DATE : 5 May, 2022

LOT NO. : 22C07

QUALITY CONTROL NO . 2 SECTION


TEST ITEM	UNIT	SPECIFICATION	RESULT
<u>EXTRACTION TEST</u>			
Limit degree of acid and alkalinity		Within 1 unit of pH	0.27
Limit of elution metal			
- Total amount of Pb, Zn , Fe, Sn	mg/L	Not greater than 5	0.0001
- Cd	mg/L	Less than 0.1	0.0000
<u>CORROSION RESISTANCE TEST</u>			
		No Sign of corrosion	No Sign of corrosion
<u>LUBRICANT</u>	mg/cm ²	Not exceed 0.25	0.043
JUDGEMENT :		PASSED	
<p>TEST METHOD : ISO 7864 : 2016 " Sterile hypodermic needles for single use "</p> <p style="text-align: center;">ISO 9626 : 2016 " Stainless steel needles tubing for manufacture of medical devices "</p>			



Approved by :

(Ms. Phinphijit B.)

Quality Control No.2 Section Manager

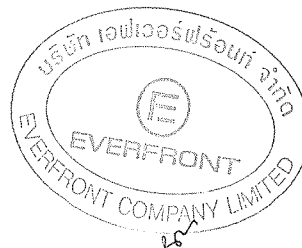



NIPRO (THAILAND) CORPORATION LIMITED
10/2 MOO 8 BANGHOMKHO, SENAPHRA NAKHON SIAYUTTHIAYA 13110, THAILAND
TEL: +66-35-201818 FAX: +66-35-201826

CERTIFICATE

PRODUCT NAME : PACK NEEDLE


SIZE : 25Gx1 1/2" LR.TW.E.P.ISO TH

DATE : 5 Aug, 2022

LOT NO. : 22E20

QUALITY CONTROL NO . 2 SECTION


TEST ITEM	UNIT	SPECIFICATION	RESULT
EXTRACTION TEST			
Limit degree of acid and alkalinity		Within 1 unit of pH	0.21
Limit of elution metal			
- Total amount of Pb, Zn, Fe, Sn	mg/L	Not greater than 5	0.0000
- Cd	mg/L	Less than 0.1	0.0000
CORROSION RESISTANCE TEST			
		No Sign of corrosion	No Sign of corrosion
LUBRICANT	mg/cm ²	Not exceed 0.25	0.048
JUDGEMENT :		PASSED	
TEST METHOD : ISO 7864 : 2016 " Sterile hypodermic needles for single use " ISO 9626 : 2016 " Stainless steel needles tubing for manufacture of medical devices "			



Approved by : _____

(Ms.Phimphijt B.)

Quality Control No.2 Section Manager

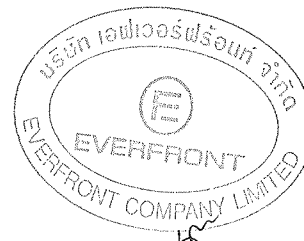



NIPRO (THAILAND) CORPORATION LIMITED
10/2 MOO 8 BANGHOM/KO,SENA,PHRA NAKH ION SIAYUTTHAYA 13110,THAILAND
TEL: +66-36-201618 FAX: +66-36-201625

CERTIFICATE

PRODUCT NAME : PACK NEEDLE


SIZE : 27Gx1/2" LR.RW.E.P.ISO TH

DATE : 5 Aug. 2022

LOT NO. : 22F16

QUALITY CONTROL NO .2 SECTION


TEST ITEM	UNIT	SPECIFICATION	RESULT
EXTRACTION TEST			
Limit degree of acid and alkalinity		Within 1 unit of pH	0.02
Limit of elution metal			
- Total amount of Pb, Zn , Fe, Sn	mg/L	Not greater than 5	0.0000
- Cd	mg/L	Less than 0.1	0.0000
CORROSION RESISTANCE TEST			
		No Sign of corrosion	No Sign of corrosion
LUBRICANT	mg/cm ²	Not exceed 0.25	0.064
JUDGEMENT :		PASSED	
TEST METHOD : ISO 7864 : 2016 " Sterile hypodermic needles for single use " ISO 9626 : 2016 " Stainless steel needles tubing for manufacture of medical devices "			

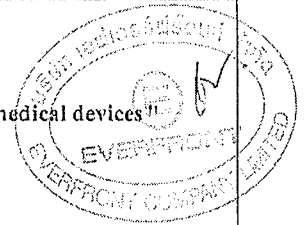

Approved by : _____

(Ms. Phimphijit B.)

Quality Control No.2 Section Manager

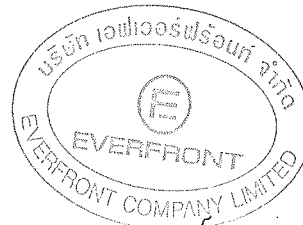



บริษัท เอส ไอ เค (ประเทศไทย) จำกัด
SIK (THAILAND) LTD.


477 ม.4 นิคมอุตสาหกรรมบางปู ซ.1 อ.สุขุมวิท ต.แพรกษา อ.เมือง จ.สมุทรปราการ 10280 โทร. 0-2709-3556 (-62), 0-2324-1051 (-55) แฟกซ์ : 0-2324-0813
477 MOO4 BANGPOO INDUSTRIAL ESTATE, SOI 1 SUKHUMVIT ROAD, PRAKSA, MUANG, SAMUTPRAKARN 10280 TEL. 0-2709-3556 (-62), 0-2324-1051 (-55) FAX : 0-2324-0813

DATE: 11 / 8 / 05

CERTIFICATE OF ANALYSIS

RESIN	PP
GRADE	P700J
COLOR CODE	1FA 571A P
LOT NO.	1E 5055
QTY (Kg)	9910 kg
Production date	15-8-05

A	COLOR	BETWEEN STD AND LIMIT PLATE	OK
B	DISPERSION		OK
C	CONTAMINATION	Φ SIZE(mm)	SPEC(pcs)
		≥ 0.5	0
		0.5-0.2	≤ 1
		0.2-0.1	≤ 2
	≤ 0.1	Conspicuous defect	OK
D	PELLET SIZE	$2.5 \Phi \pm 0.5\text{mm} \times 3.0 L \pm 0.5\text{mm}$	OK
E	PELLET	No abnormal shall be recognized in pellet	OK
F	MOISTURE	No moisture shall be recognized in pellet or silver streak in plate	OK

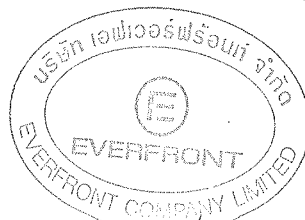

QC MANAGER



PA-OB PITUCKCHANUAN



บริษัท เอส ไอ เค (ประเทศไทย) จำกัด
SIK (THAILAND) LTD.


477 ม.4 นิคมอุตสาหกรรมบางปู ซ.1 ต.สุขุมวิท ต.แพรกษา อ.เมือง จ.สมุทรปราการ 10280 โทร. 0-2709-3556 (-62), 0-2324-1051 (-55) แฟกซ์ : 0-2324-0813
477 MOO 4 BANGPOO INDUSTRIAL ESTATE, SOI 1 SUKHUMVIT ROAD, PRAKSA, MUANG, SAMUTPRAKARN 10280 TEL. 0-2709-3556 (-62), 0-2324-1051 (-55) FAX : 0-2324-0813

DATE: 4 / 8 / 05

CERTIFICATE OF ANALYSIS

RESIN	PP
GRADE	P402J
COLOR CODE	TBA Δ719P-TP
LOT NO.	TE 0176
QTY (Kg)	2,000 Kg
Production date	3/8/05


A	COLOR	BETWEEN STD AND LIMIT PLATE	OK
B	DISPERSION		OK
C	CONTAMINATION	Φ SIZE(mm)	SPEC(pcs)
		≥ 0.5	0
		0.5-0.2	≤ 1
		0.2-0.1	≤ 2
	≤ 0.1	Conspicuous defect	OK
D	PELLET SIZE	2.5 Φ ± 0.5mm x 3.0 L ± 0.5mm	OK
E	PELLET	No abnormal shall be recognized in pellet	OK
F	MOISTURE	No moisture shall be recognized in pellet or silver streak in plate	OK



QC MANAGER



PA-OB PITUCKCHANUAN

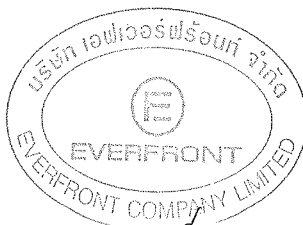

INSPECTION RESULT FOR POLYMER CHIP

QCI NO. AC-01-PS:0508-06



ITEM NO.	NAME & CODE	LOT NO.	VISUAL RESULT FROM 1,000 g						WEIGHT OF 10 pcs.(g)						JUDGE MENT	
			COLOR	FM	ST	AB	TH	TOTAL	1	2	3	4	X	R		
				(pcs.)	(pcs.)	(pcs.)	(pcs.)	(g)								
1	PP P750J	8E190276	NATURAL	0	0	0	0	0	0.20	0.20	0.19	0.20	0.20	0.01	(AC)	RE
		8E310448	NATURAL	0	0	0	0	0	0.19	0.20	0.19	0.19	0.19	0.01	(AC)	RE
2	PP P700J	8F309505	NATURAL	0	0	0	0	0	0.19	0.18	0.18	0.19	0.18	0.01	(AC)	RE
3	PP AR564 KFC-8A825	57D2006	LGREEN	0	0	0	0	0	0.17	0.16	0.17	0.17	0.17	0.01	(AC)	RE
4	PP AR564 KFC-4B173	57D2005	RED	0	0	0	0	0	0.15	0.14	0.14	0.14	0.14	0.01	(AC)	RE
5	PP P700J TFA5719P	7E5174	Blue	0	0	0	0	0	0.11	0.11	0.11	0.10	0.11	0.01	(AC)	RE
6	PP P702J TBA4719P-TP	7E5176	Pink	0	0	0	0	0	0.14	0.15	0.15	0.15	0.15	0.01	(AC)	RE
REMARK :																

SPECIFICATION.

ITEM	TYPE	PP	PS	PE	PC	POM	ABS	ELAS	MILAS
FOREIGN MATTER (FM)		10	10	10	10	10	10	10	10
STICK (ST)		20	0	0	0	0	0	0	0
ABNORMAL SHAPE (AB)		0	0	0	0	0	0	0	0
THREAD (TH)		40	0	0	0	0	0	0	0

Inspected by	Confirmed by
Sonthaya 06 Aug, 05	<i>[Signature]</i> 06 Aug, 05

Executed on 04 Jul, 05

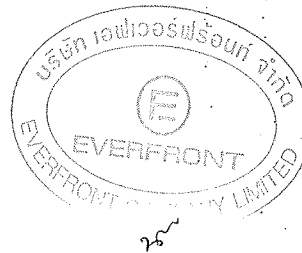

b/6

24871-73053-1



The Polyolefin Company (Singapore) Pte. Ltd.

Office : 150 Beach Road, #10-00 Gateway West, Singapore 189720
Tel: (65) 6292 9622 Fax: (65) 6293 8890, (65) 6292 6595, (65) 6293 2748
Plant : #01 Ayer Merbau Road, Singapore 628285
Website: www.tpc.com.sg Co. Reg. No.: 198001666D

Certificate of Analysis

Date 23-MARCH-2005
Customer Name NIPRO (THAILAND) CORPORATION LIMITED
Contract Number CTH3063070
Vessel Name / Voyage No. GANTA BHUM / 110E
ETD 24-MARCH-2005
Customer P/O No. 74-IKS-090448
L/C No. -

We, the manufacturer of the undermentioned products, hereby certify that the undermentioned products have been duly inspected by us and in conformity with our product specifications.

Product : POLYPROPYLENE
Brand : COSMOPLENE
Grade : FF9014



LOT NUMBER		GUB207
QUANTITY		16.0 MT
PHYSICAL PROPERTY	UNIT	
CONTAMINATION	NO/100G	0
DENSITY WITH FIXED VALUE	G/CM3	0.9
MELT FLOW RATE	G/10MIN	18.60
YELLOWNESS INDEX		-2.9

Remarks

THE POLYOLEFIN COMPANY
(SINGAPORE) PTE LTD

Brian Tan Bah Ean
Sales Manager
Sales & Marketing

WITHIN
04/31 Mar, 05
SPECIFICATION

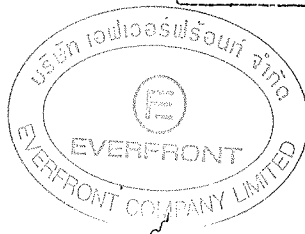

16

INSPECTION RESULT FOR POLYMER CHIP

OCI NO. AC:01.PS:0504-01



ITEM NO.	NAME & CODE	LOT NO.	VISUAL RESULT FROM 1,000 g						WEIGHT OF 10 pcs.(g)						JUDGE MENT		
			COLOR	FM (pcs.)	ST (pcs.)	AB (pcs.)	TH (pcs.)	TOTAL (g)	1	2	3	4	X	R			
1	PP FF9014	GUB207	NATURAL	0	0	0	0	0	0.21	0.20	0.20	0.20	0.20	0.01	AC	RE	
2	ABS DENKA QFT	0412129-CB	NATURAL	0	0	0	0	0	0.18	0.18	0.17	0.19	0.18	0.01	AC	RE	
		0412137-CB	NATURAL	0	0	0	0	0	0.15	0.16	0.15	0.15	0.15	0.01	AC	RE	
		0501287-CB	NATURAL	0	0	0	0	0	0.15	0.15	0.15	0.16	0.15	0.01	AC	RE	
															AC	RE	
																AC	RE
																AC	RE
REMARK ;																	

SPECIFICATION.

ITEM	TYPE	PP	PS	PE	PC	POM	ABS	ELAS	MILAS
FOREIGN MATTER (FM)		10	10	10	10	10	10	10	10
STICK (ST)		20	0	0	0	0	0	0	0
ABNORMAL SHAPE (AB)		0	0	0	0	0	0	0	0
THREAD (TH)		40	0	0	0	0	0	0	0

Inspector by	Confirmed by	Approved by
SORNHAYA 01 APR, 05	<i>[Signature]</i> 01 APR, 05	<i>[Signature]</i> 01 APR, 05

Executed on 22 Dec., 04

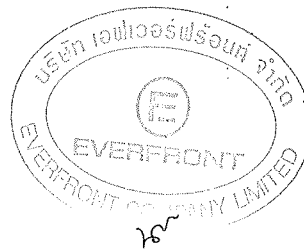



บริษัท โอเร็กซ์ เทรดดิ้ง จำกัด
OREX TRADING COMPANY LIMITED

126 ซอยเรวัติ 14 ตำบลตลาดขวัญ อำเภอเมืองนนทบุรี จังหวัดนนทบุรี 11000
Tel : (662) 977-9444 (12 Lines) , (662) 977-9333 (12 Lines) Fax : (662) 977-9343 , (662) 977-9373
126 Soi Raewadee 14, Talad Khuan, Nonthaburi 11000, Thailand. E-mail : orex@orex.co.th

หนังสือแต่งตั้งตัวแทนจำหน่าย

วันที่ 3 พฤษภาคม 2566

บริษัท โอเร็กซ์ เทรดดิ้ง จำกัด สำนักงานตั้งอยู่เลขที่ 126 ซอยเรวัติ 14 ตำบลตลาดขวัญ อำเภอเมืองนนทบุรี จังหวัดนนทบุรี 11000 ผู้แทนจำหน่าย “NIPRO” เข็มฉีดยา (Disposable Needle) ในประเทศไทย อนุญาตและแต่งตั้งให้

บริษัท เอฟเวอร์ฟรอนท์ จำกัด
เลขที่ 126 ซอยเรวัติ 14 ตำบลตลาดขวัญ
อำเภอเมืองนนทบุรี จังหวัดนนทบุรี 11000
ทะเบียนนิติบุคคลเลขที่ 0125566010422

เป็นตัวแทนจำหน่าย “NIPRO” เข็มฉีดยา (Disposable Needle) เบอร์ 16G x 1.1/2", 18G x 1" , 18G x 1.1/2" , 20G x 1" , 20G x 1.1/2" , 21G x 1" , 21G x 1.1/2" , 22G x 1" , 22G x 1.1/4" , 22G x 1.1/2" , 23G x 1" , 23G x 1.1/4" , 23G x 1.1/2" , 24G x 1" , 24G x 1.1/4" , 24G x 1.1/2" , 25G x 5/8" , 25G x 1" , 25G x 1.1/2" , 26G x 1/2" , 26G x 1" , 27G x 1/2" และ 27G x 1"



ทั้งนี้ มีระยะเวลาตั้งแต่บัดนี้ไปจนถึงวันที่ 31 ธันวาคม 2566



บริษัท โอเร็กซ์ เทรดดิ้ง จำกัด

(นายชาติรี สุขสำราญ)

ผู้จัดการฝ่ายขายและการตลาด

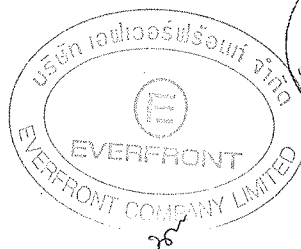



NIPRO SALES (THAILAND) COMPANY LIMITED
33/170 Nipro Building, Viphavadee Rangsit Road,
Talad Bangkhen, Laksi, Bangkok 10210 Thailand.
Tel : +66 2551 2000 Fax : +66 2551 2005

Date: 1st March 2023

AUTHORIZATION LETTER

To Whom It May Concern:

NIPRO SALES (THAILAND) COMPANY LIMITED is the company registered at
Address: 89/170 Nipro Building, Viphavadee Rangsit Road,
Talad Bangkhen, Laksi, Bangkok 10210 Thailand

Hereby certify that:

OREX TRADING COMPANY LIMITED



Address: 126 Soi Rawadee 14, Talad Khuan, Nonthaburi District, Nonthaburi 11000 Thailand
Tel: (66) 0 2977 9444
Fax: (66) 0 2977 9343

Is the Authorized Distributor in Thailand for the groups of product indicated hereunder;


- NIPRO Disposable Needle (All sizes, excluding 18G x 3/4", 20G x 1/2" and 30G x 1/2")
- NIPRO Disposable Syringe with Needle (3, 5, 10 mL)
- NIPRO Disposable Syringe Insulin 1 mL (26G, 27G, 29G)
- NIPRO Disposable Syringe Insulin 0.3, 0.5 and 1 mL (30G x 1/2", 30G x 5/16")
- NIPRO Disposable Syringe TB 1 mL (All sizes, excluding 1 mL, 25G x 5/8")
- NIPRO Disposable Syringe without Needle (1, 3, 5, 10, 20, 50 mL)
- NIPRO Scalp Vein Set (All sizes)
- NIPRO Infusion Set
- NIPRO Extension Tube
- NIPRO I.V. Catheter (Safelet Cath)
- NIPRO 3-Way Stopcock
- NIPRO Disposable SafeTouch PSV
- NIPRO Disposable SafeTouch IV Cath
- NIPRO Premier α (Alpha)
- NIPRO Premier S (Standard)
- NIPRO Premier Test Strip (10CT, 25CT, 50CT)
- NIPRO Premier Glucose Control Solution (H&L, H, M, L Pack)
- CareSens Lancet 28G, 30G
- NIPRO Spinal Needle

This authorization letter is valid until March 31st, 2024.

Yours Faithfully



Mr. Junya Sato
President
Nipro Sales (Thailand) Co., Ltd.

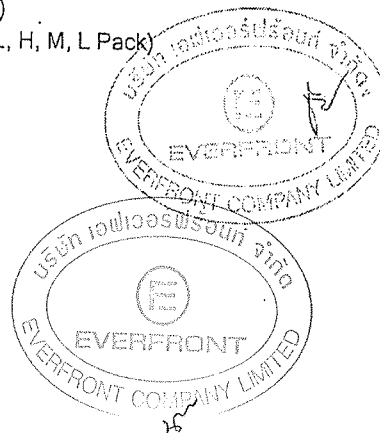



NIPRO (THAILAND) CORPORATION LIMITED

10/2 MOO 8 BANGNOMKO, SENA, PHRA NAKHON SI AYUTTHAYA 13110, THAILAND
TEL. (035) 20-1618-1624 FAX: (035) 20-1625, (035) 20-1627

Date : January 31st 2017

AUTHORIZED LETTER

TO : WHOM IT MAY CONCERN



NIPRO (THAILAND) CORPORATION LIMITED is the company registered at
Address: 10/2 Moo 8, Bangnomko, Sena, Phra Nakhon Si Ayutthaya, 13110, Thailand

Hereby certifies the following company:

NIPRO SALES (THAILAND) COMPANY LIMITED
Address : 2nd Floor, Juthamard Building, 89/170 , Viphavadee Rangsit Road,
Talat Bangkhen, Laksi, Bangkok 10210 Thailand
Tel : (662) 551-2000

is the Authorized Distributor of Nipro (Thailand) Corporation Limited.

This authorized letter valid from the above date till further notice.

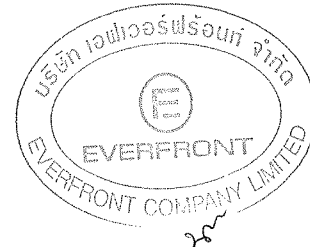


Yours Faithfully,

Mr. Yoshiharu Yonemori
President
Nipro (Thailand) Corporation Limited




หนังสือมอบอำนาจ

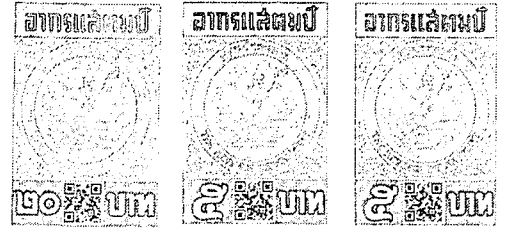

วันที่ 3 สิงหาคม 2566

ข้าพเจ้า บริษัท เอฟเวอร์ฟรอนท์ จำกัด ทะเบียนนิติบุคคลเลขที่ 0125566010422 เมื่อวันที่ 14 มีนาคม 2566 โดยนายสวัสดิ์ ดอนสกุล กรรมการผู้จัดการบริษัท ขอมอบอำนาจให้ นายชาติร์ สุขสำราญ เป็นผู้ที่มีอำนาจยื่นขอ เปิดซอง เสนอราคา , ประกวดราคา , ตีซองราคา และแก้ไขเอกสาร ประกวดราคาซื้อ วัสดุการแพทย์ (เข็มฉีดยาปราศจากเชื้อ) จำนวน 13 รายการ ด้วยวิธีประกวดราคาอิเล็กทรอนิกส์ (e-bidding) ตามประกาศจังหวัดนครปฐม (โรงพยาบาลนครปฐม) เอกสารประกวดราคาซื้อด้วยวิธีประกวดราคาอิเล็กทรอนิกส์ (e-bidding) เลขที่ 73/2566 ลงวันที่ 21 กรกฎาคม 2566

การใดๆ ที่ นายชาติร์ สุขสำราญ ผู้รับมอบอำนาจได้กระทำไปในขอบเขตข้างต้น ให้มีผลเสมือนหนึ่ง เป็นการกระทำของบริษัท และบริษัทขอรับผิดชอบทุกประการ เพื่อเป็นหลักฐานผู้มอบและผู้รับมอบอำนาจต่างได้ ลงลายมือชื่อไว้เป็นสำคัญ




ลงชื่อ ผู้มอบอำนาจ
(นายสวัสดิ์ ดอนสกุล)

ลงชื่อ ผู้รับมอบอำนาจ
(นายชาติร์ สุขสำราญ)

ลงชื่อ พยาน
(นางสาวอังคณา เหมน้อย)

ลงชื่อ พยาน
(นางสาวสุนันทา สนวนสมุทร)

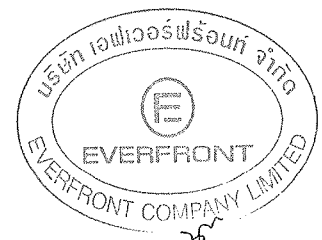

รายการเดินบัญชีเงินฝากกระแสรายวัน (มีรายละเอียด)

开泰往来账户对账单 (附明细) K-DEPOSIT STATEMENT OF CURRENT ACCOUNT (WITH DETAIL)

ธนาคารกสิกรไทย
开泰银行 KASIKORNBANK



ที่ DD.047 : N230518135100741257830/2566

หน้าที่ 1/1 (0465)

ชื่อบัญชี บริษัท เอฟเวอร์ฟรอนท์ จำกัด

126 ซ.เรวดี 14 ต.ตลาดขวัญ อ.เมือง จ.นนทบุรี 11000

เลขที่อ้างอิง	23051813510074125783
เลขที่บัญชีเงินฝาก	XXX-X-XX741-8
รอบระหว่างวันที่	20/04/2023 - 17/05/2023
สาขาเจ้าของบัญชี	สาขาศิวานนท์ 8

บริษัท เอฟเวอร์ฟรอนท์ จำกัด

ธนาคารกสิกรไทย จำกัด (มหาชน) สาขา ศิวานนท์ 8

บัญชีกระแสรายวัน เลขที่บัญชี 155-2-98741-8

รับรองสำเนาถูกต้อง

(นายสวัสดิ์ ดอนสกุล)

